

EXTERNAL IMAGING GUIDE

1. BEFORE YOU BEGIN, PULL THE NONMYD ALPHA ALL THE WAY BACK TO AVOID HAVING THE PATIENT HIT THE OBJECTIVE LENS WITH THEIR NOSE.





2. PULL THE DIOPTRIC COMPENSATION KNOB ALL THE WAY OUT.

3. TURN OFF THE GREEN INDICATOR LIGHT IN FRONT OF THE JOYSTICK.



4. CHOOSE THE FIELD OF VIEW YOU WISH TO CAPTURE AT (45 DEGREES WORKS BEST).

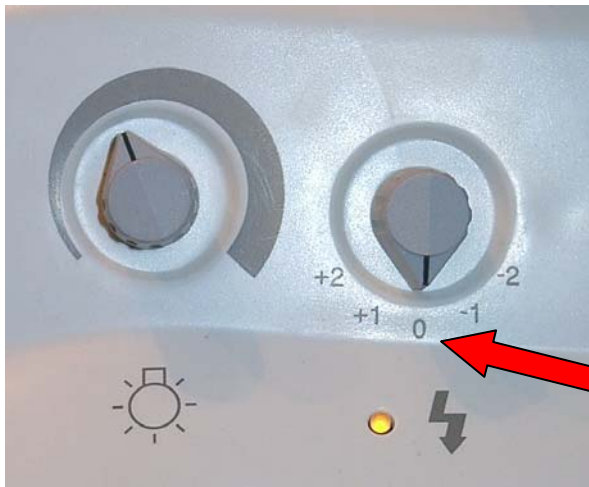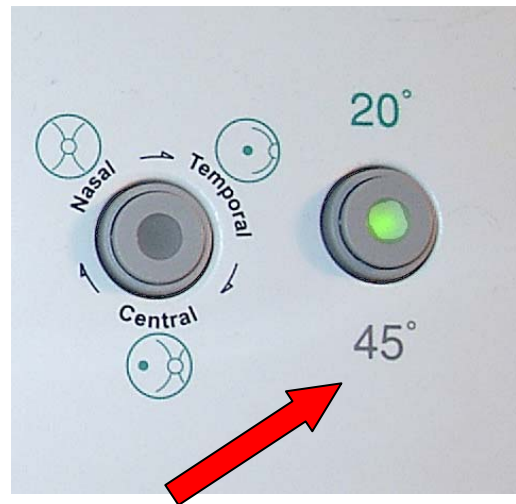

5. START WITH THE FLASH SETTING AT "0" AND THE BLUE / BROWN SWITCH SET TO BROWN.

